

## Exploring the Potentials of Asphalt Solar Collectors in Hot Humid Climates

Khoja AO<sup>1</sup> and Waheeb SA<sup>2\*</sup>

<sup>1</sup>Munich University of Applied Sciences, München, Germany

<sup>2</sup>Umm AlQura University, Makkah, Saudi Arabia

\*Corresponding author: Sahl Abdullah Waheeb, Umm AlQura University, Makkah, Saudi Arabia, Tel: +966555690755; E-mail: [Sawaheeb@gmail.com](mailto:Sawaheeb@gmail.com)

Received date: July 30, 2016; Accepted date: September 17, 2016; Published date: September 19, 2016

Copyright: © 2016 Khoja AO, et al. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

### Abstract

To date, research on possible applications of asphalt solar collector technology (ASC) has been focused on their usage of in cold to moderate climate conditions, mostly for road de-icing and heat pumps. Both of these applications require large and expensive intercessional heat storage units. This paper will explore potential applications of ASC in hot and humid climates by evaluating the performance of a simulated 20 m<sup>2</sup>ASC meeting the demand of three low to medium-temperature solar thermal applications, namely: solar assisted cooling, atmospheric water generation and domestic hot water.

**Keywords:** Asphalt solar collectors; Solar assisted cooling; Atmospheric water generation; Jeddah; Saudi Arabia

[2]. Thus, ASC can be relatively easily integrated in the current infrastructure without a negative impact on the structural performance of paved roads [3,4].

### Introduction

Asphalt solar collectors (ASC) involve the use of asphalt-paved surfaces to harvest solar energy. ASC is a relatively new technology that has become a research focus in the past few years due to the thermal properties of asphalt and the abundance of asphalt infrastructure in modern cities, as 35–60% of modern cities are already paved with asphalt [1] and resurfaced, on average, every 12–20 years

An ASC system consists of a pipe embedded in the wearing course of asphalt pavement, which acts as a heat exchanger (Figure 1). ASC systems function by pumping fluid through the embedded pipe. The fluid temperature rises as it collects the heat from the asphalt pavement. The heated fluid is then collected in storage tanks for further use.

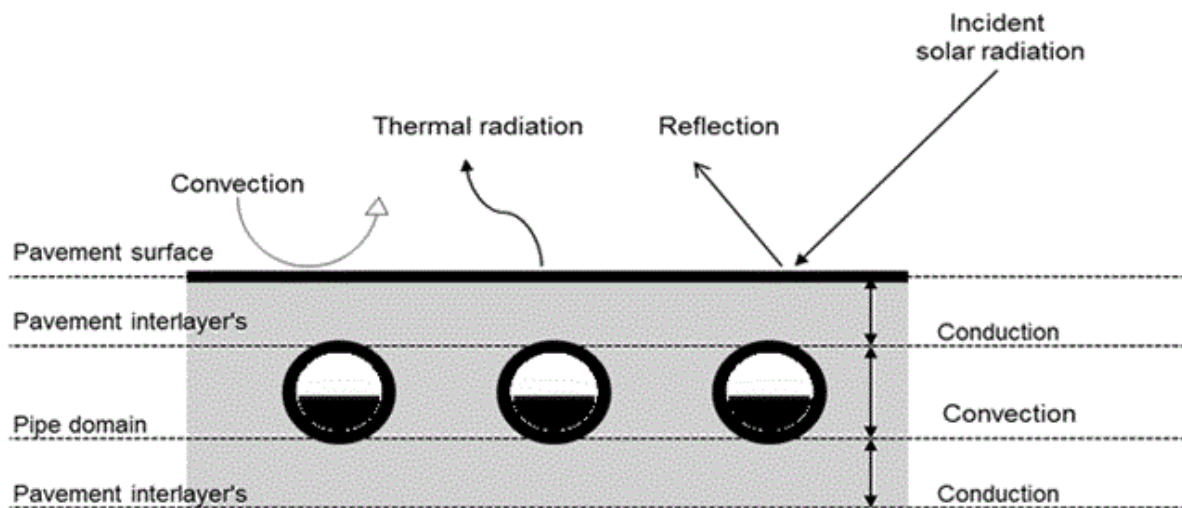


Figure 1: Heat transfer mechanisms in an ASC.

### Methodology

The presented research is conducted with the help of the numerical simulation software TRNSYS. The typical meteorological year (TYR)

weather data of the city of Jeddah, Saudi Arabia was chosen for this research as its climactic conditions reflect those of a typical hot and humid climate, characterized by hot to extremely hot summers and mild to warm winters. Rain is scarce with minimal cloud cover. TYR

weather data show that temperature and solar radiation intensity reach their maximums during the summer months between May and September with minimum cloud cover and almost no rain.

Simulation frame	time	Pumping regime	Inlet temperature	water	Asphalt area
From 1st of APR to 30th SEP with a 1 min time step		From sunrise to sunset	Mains temperature from weather file	water TYR	20 m <sup>2</sup>

**Table 1:** Summary of the simulation boundary conditions.


This research was conducted during this period of the year as it is during this time that ASC performance is expected to reach its peak. In Table 1, a summary of the simulation boundary conditions is provided.

To ensure the reliability of the simulated model, the asphalt pavement is modelled in TRNSYS using the same thermal and physical properties of a real sample from the case study site (Table 2) [5].

Layer	Thickness [m]	Thermal conductivity [W/m <sup>2</sup> K]	Heat capacity [kJ/kg/K]	Density [kg/m <sup>3</sup> ]
Wearing course	0.05	2.5	1	2300
Base course	0.08	1.8	1.1	2200
Sub-base course	0.25	1.8	0.9	2200
Sub-grade course	30	1.5	0.85	1500

**Table 2:** Asphalt properties as found in Alawi [5] study and used to build the ASC model in TRNSYS.

A comparison between the thermal behaviour of the modelled asphalt against the real one is carried out to insure that the modelled sample behaves similarly to the real one (Figure 2).

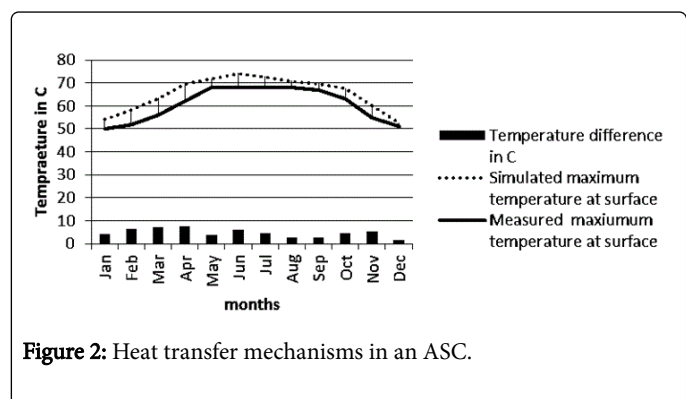

**Figure 2:** Heat transfer mechanisms in an ASC.

The comparison results showed a general agreement in thermal behaviour between the simulated and real samples [5] as well as with the Saudi Arabia asphalt grade recommendation map [6], with results indicating that the sample can safely be considered valid for the purposes of this research. The difference in temperature between the simulated and measured surfaces was an average of 5K. This difference can be attributed to a number of factors, such as the fact that the

simulations are based on TYR weather data and not on real time weather data.

An optimized configuration of the ASC components was developed. ASC system components along with the asphalt thermal properties are chosen based on information in previously published articles on the topic [7-9] with the addition of the road rated insulation Styrodur<sup>®</sup>C 4000 CS, with of conductivity ( $\lambda$ )=0.032 W/m<sup>2</sup>K [10]. A sensitivity analysis was performed on the asphalt pavement and heat exchangers in order to develop an optimized ASC model to yield the largest amount of useful energy for low to medium temperature solar thermal applications. ASC optimization is achieved by assessing the impact of each ASC system component on the performance of the ASC as per the following criteria

1. The amount of fluid collected at temperatures between 45°C and 55°C at 2.5K intervals along the simulation time frame
2. The maximum temperature reached by the fluid at the outlet.
3. The maximum temperature difference between the inlet and outlet.
4. The collected heat by the ASC  $Q_c = (V \times C_p \times \Delta T) / A_{(ASC)}$  [W/m<sup>2</sup>] (1).
5. The system efficiency,  $\eta = (\text{heat collected by ASC}) / (\text{solar radiation on ASC})$  [%] (2).

A summary of the investigated variables of the ASC is displayed in (Tables 3 and 4).

Wearing conductivity ( $\lambda$ ) [W/m <sup>2</sup> K]	Insulation thickens [cm]	Insulation depth from surface [cm]	Wearing heat capacity (C) [kJ/kg/K]
2	3	0	0.9
2.5	4	5	1
2.88	5	13	1.1

**Table 3:** Investigated asphalt wearing course thermal properties.

Pipe material $\lambda$ [W/m <sup>2</sup> K]	Pipe spacing [cm]	Pipe depth [cm]	Pipe diameter [cm]
Copper [401]	10	3	1
PEX [0.47]	15	4	2
PVC [0.19]	20	5	3

**Table 4:** Investigated ASC heat exchanger properties.

Supporting components such as the storage tank, power source and a pump were added to the ASC system in order to achieve full functionality. These supporting systems were chosen from commercially available devices to allow for further validation of the simulation results on a field test as well as for assessing the overall performance of complete ASC system under real life conditions.

### Water Tank Properties

A vertical insulated hot water tank was used in the simulation. The tank height was 2 m and its capacity was 3 m<sup>3</sup>. Its heat loss coefficient value was 0.1 [W/m<sup>2</sup>×K].

### Water Pump Properties

A direct current (DC) water pump with a rated capacity of 1000 kg/h was used. The main advantages of the DC pump are its high efficiency and the fact that the pump can be directly wired to a PV panel without the need of an additional DC/AC converter, as the ASC system is expected to work in phase with sun radiation intensity, rendering the use of a backup battery unnecessary.

Pump	Pump type	Rated voltage	Rated power	Max flow rate	Max head
Specifications	Centrifugal	12 [V] DC	13 [W]	1020 [L/h]	2 [m]

Table 5: Specifications of the water pump [11].

### Photovoltaic Panel Properties

A 12v 30WP photovoltaic panel was chosen as the power source for the pump. The PV panel was installed facing the horizontal radiation, as this angle is the optimum angle for PV panels during the summer months in Jeddah [12:48] and the working hours of the pump.

PV	PV type	Peak power	Cells number	Efficiency
Specifications	Monocrystalline	30 [WP]	36	16.1 [%]

Table 6: Specification of the PV panel [13].

The performance of the developed ASC is to be evaluated based on assessing the ASC's ability to meet the load demand of three solar thermal applications, which are:

1. A 2 kW absorption solar cooling (AC) unit
2. An atmospheric water generator (AWG) with a water extraction efficiency of 35% [14]
3. A domestic hot water demand (DHW) of 600 L/day which represents the daily consumption of about 10 persons [15].

Application	Minimum driving temperature	Maximum driving temperature	Load time profile	$\Delta T$ supply & return temperature
AC	65C	N/A	9am-6pm	5K [16]
AWG	60C	N/A	2pm-8am	5K
DHW	55C	60C	20pm-21pm	N/A

Table 7: Specifications of the water pump [11].

The maximum and minimum driving temperatures of each system are specified based on the published working temperature of each system [14,17,18].

The AC load hours are chosen between 9am and 6pm as they match the typical cooling demand load profile, where the AWG load hours are chosen between 2am and 8am. During this time, the relative humidity is at its highest, thus allowing the system to extract the largest possible amount of water from the air. ASC system performance meeting each load is evaluated based on the following criteria

1. The ASC system working hours

2. The amount of water collected above the minimum driving temperature
3. The collected heat by the ASC,  $q=(V \times C_p \times \Delta T)/A-(ASC)$  [W/m<sup>2</sup>] (1)
4. The system efficiency,  $\eta=(\text{heat collected by ASC})/(\text{solar radiation on ASC})$  [%] (2)
5. The system working fraction,  $f=((\text{working hours})/(\text{load hours}) \times 100)$  [%] (3).

An air-to-water heat exchanger was used to mimic the effects of the load of each of the three applications on the return water temperature to the storage tank. This type of heat exchanger was used due to it being a stable system that can be easily specified and controlled, and can thus be easily integrated into further field tests performed under real conditions. Heat exchanger performance was calculated separately for each of the scenarios using the Number of Transfer Units Effectiveness Method (NTU) [16].

The NTU value was used in order to regulate the amount of heat extracted from the water by the heat exchanger in order to deliver the return water from the heat exchanger to the tank at the correct temperature as if the water was subjected to real load. The temperature of the return water in the AWG and AC applications is taken from [14,18] respectively. A schematic of the developed ASC system is provided (Figure 3).

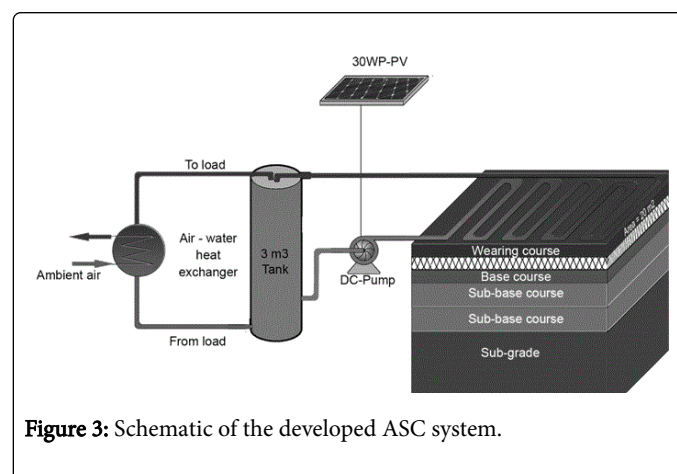


Figure 3: Schematic of the developed ASC system.

### Development of the Optimized ASC Configuration

The sensitivity analysis revealed that the heat insulation and asphalt heat capacity had the most positive impacts on temperature difference between the fluid inlet and outlet temperatures.

Asphalt	Thickness [m]	Thermal properties		
		$\lambda$ [W/m×K]	C [kJ/kg/K]	$\rho$ [kg/m <sup>3</sup> ]
Wearing	0.05	2.5	0.9	2300
Insulation	0.03	0.032	1.47	38

Table 8: Asphalt properties of the optimized ASC model.

On the other hand, increasing the system depth had the most negative impact, followed by increasing the pipe spacing. Asphalt conductivity and solar absorption showed very little correlation with system performance.

Increasing heat insulation thickness made a slight impact on system performance. Properties of the ASC optimized system are specified in (Tables 8 and 9).

Pipes depth[m]	Pipe $\lambda$ [W/m $\times$ K]	Flow rate [kg/h]	Pipe geometry		
			Spacing [m]	Diameter [m]	Thickness [m]
0.03	0.47	875	0.1	0.02	0.002

Table 9: Heat exchanger properties of the optimized ASC model.

Month	Average Tank Temperature [°C]	System working hours [h]	System working fraction 270 working hours/month [%]	Water collected above min driving temperature [Liter/m <sup>2</sup> ]	Average efficiency [%]	Average heat gain [kW/m <sup>2</sup> ]
May	64.71	90.85	33.65	2491.56	12.13	110.71
June	64.7	51.58	19.10	1836.77	9.58	87.97
July	64.86	82.93	30.72	2191.88	12.34	102.31
August	64.84	87.87	32.54	2341.35	13.39	100.1
September	64.78	53.17	19.69	1789.38	10.54	87.2

Table 10: Performance of the optimized ASC meeting the load of the 2 kW Absorption solar cooling (AC).

Month	Average Tank Temperature [°C]	System working hours [h]	System working fraction (180 hours/month) [%]	Water collected in above minimum driving temperature [Liter/m <sup>2</sup> ]	Amount of generated water [Liter/m <sup>2</sup> ]	Average system efficiency [%]	Average heat gain [kW/m <sup>2</sup> ]
May	62.05	162.98	90.55	3502.19	57.99	16.15	148.02
June	61.22	145.9	81.06	3067.6	54.27	14.86	136.6
July	61.94	167.27	92.93	3278.33	64.15	17.03	140.09
August	62.01	168.27	93.48	3676.46	75.82	19.42	144.92
September	61.3	149.07	82.81	3146.35	66.07	16.75	139.89

Table 11: Performance of the optimized ASC meeting the load of an atmospheric water generator (AWG) with a water extraction efficiency of 35%.

Month	Average tank temperature [°C]	System working hours [h]	System working fraction (30 hours / month) [%]	Water collected above minimum driving temperature [Liter/m <sup>2</sup> ]	Average system efficiency [%]	Average heat gain [kW/m <sup>2</sup> ]
May	60.06	58	97	3028.23	21.97	198.39
June	59.19	49.93	83	2945.83	20.07	183.97
July	59.63	54.47	91	2879.48	22.25	181.8
August	59.32	58.03	97	3162.4	24.62	191.35
September	59.02	48.9	82	2923.23	23.66	193.21

Table 12: Performance of the optimized ASC meeting the load of 600 L/day of domestic hot water (DHW).

## Results

The results of investigating ASC performance under the three loads are promising (Tables 10-12).

In general, the system showed potential for atmospheric water generation and meeting the domestic hot water load, with the former being of high importance, especially in hot humid climate conditions. In the month of August, working under the load of DHW, The 20 m<sup>2</sup> ASC system extracted 1516 litres of water from the air and reached an average efficiency of almost 25%.

## Conclusion and Discussion

This paper has investigated the performance of ASC in hot humid climates by means of simulation with TRNSYS [16]. The performance of the simulated asphalt pavement model is provisionally validated against empirical data from the case study city in order to ensure the reliability of the created TRNSYS model.

The optimized asphalt solar collector along with its necessary supporting components was developed based on a sensitivity analysis and the availability of commercial devices in order to facilitate the building of a real system based on the given specifications for further field tests to validate the research results. The results of the sensitivity analysis indicate that the addition of a road-rated heat insulation layer below the pipe-carrying asphalt layer has improved ASC performance. The results of the sensitivity analysis indicate that, in general, the heat components of the ASC (pipes and fluid) have a greater influence on the performance of the ASC system than the asphalt properties do. The main ASC design components that were found to impact the performance of the ASC, with respect to achieving the highest temperature difference between the fluid inlet and outlet were the fluid flow rate, the fluid heat capacity and the depth of the heat exchanger system, in that order.

The performance of the developed system was analyzed and evaluated under the load of an absorption cooling cycle, an atmospheric water generator and typical domestic hot water demand between the months of May and September. ASC performance for the above mentioned solar thermal applications indicate a strong potential for the use of the ASC technology to cover domestic hot water demand as well as for atmospheric water generation, with the latter being of especially high importance in hot and humid climates where there is an abundance of asphalt paved roads. It should be noted that designing a specified load for each of the previously-mentioned cases was beyond the scope of this research. Therefore, the results of this research should be considered accordingly.

## Implications for Future Research

The results of this paper are relevant to understanding the potential applications of ASC technology in hot, arid climates. It has been demonstrated that ASC is a viable technology for arid, urban environments. The results of this study indicate a need for further field tests in different weather conditions in order to accurately assess the applicability of ASC systems to meet such demands as well as to validate the results of this research.

Preliminary cost estimates from local contractors for the proposed additions to the normal paving for the ASC system represent an extra 25\$ per m<sup>2</sup>. A cost-benefit analysis and the potential applicability of combining ASC with other solar energy harvesting systems were not part of this research. An analysis of the impact of the system on the

safety and durability of paved roads should be included in future field test research.

Overall, the results of this research imply a wide array of potential applications for ASC technology, demonstrate the validity of the new technology, and indicate a need for further field test research.

## References

1. Akbari H, Rose LS, Taha H (2003) Analyzing the land cover of an urban environment using high-resolution orthophotos. *Landsc Urban Plan* 63: 1-14.
2. National Cooperative Highway Research Program (2011) A manual for design of hot mix asphalt with commentary. Transportation Research Board 673.
3. Sheeba BJ, Rohini AK (2014) Structural and thermal analysis of asphalt solar collector using finite element method. *Journal of Energy*.
4. Carder DR, Barker KJ, Hewitt MG, Ritter D, Kiff A (2008) Performance of an interseasonal heat transfer facility for collection, storage, and re-use of solar heat from the road surface. TRL Published Project Report.
5. Alawi MH, Helal MM (2014) A mathematical model for the distribution of heat through pavement layers in Makkah roads. *Journal of King Saud University-Engineering Sciences* 26: 41-48.
6. Wahhab HAA, Ali MF, Asi IM, Al-Dubabe IA (1995) Adaptation of shrp performance based binder specifications to the gulf countries.
7. Bobes-Jesus V, Pascual-Muñoz P, Castro-Fresno D, Rodriguez-Hernandez J (2013) Asphalt solar collectors: a literature review. *Applied Energy* 102: 962-970.
8. Mallick RB, Chen BL, Bhowmick S, Hulen M (2008) Capturing solar energy from asphalt pavements. In *International symposium on asphalt pavements and environment, international society for asphalt pavements, Zurich, Switzerland*.
9. Shaopeng W, Mingyu C, Jizhe Z (2011) Laboratory investigation into thermal response of asphalt pavements as solar collector by application of small-scale slabs. *Applied Thermal Engineering* 31: 1582-1587.
10. Se B (2013) Technical data recommended applications assistance data for dimensioning.
11. Hierner GmbH (2009).
12. Tan A, Maerten M (2011) Cooling system for solar housing in the Middle East: A design study based on a concept.
13. CNPV-Power (2013).
14. Wahlgren RV (2001) Atmospheric water vapour processor designs for potable water production: a review. *Water Research* 35: 1-22.
15. Meyer J (2000) A review of domestic hot water consumption in South Africa. *R&D Journal* 16: 55-61.
16. Shah RK, Sekulic DP (2003) *Fundamentals of heat exchanger design*. John Wiley & Sons.
17. World Health Organization (2011) *Guidelines for drinking-water quality*. WHO, Geneva.
18. Zhai XQ, Qu M, Li Y, Wang RZ (2011) A review for research and new design options of solar absorption cooling systems. *Renewable and Sustainable Energy Reviews* 15: 4416-4423.