

Investigation of Neutron in Linear Accelerator at Dong Nai General Hospital by Using the Neutron Activation Method

Nguyen Van Hai^{1*}, Nguyen Van Hung², Nguyen Van Hoa³ and Dao Thi Kim Nhung³

¹Dalat Vocational Training College, Vietnam

²Nuclear research Institute, Vietnam

³Health Center of Lac Duong, Vietnam

*Corresponding author: Nguyen Van Hai, Dalat Vocational Training College, 01 Hoang Van Thu Street, Ward 4, Dalat City, Lam Dong Province, Vietnam, Tel: +84913063277; E-mail: haiitdl@gmail.com

Received date: Mar 10, 2015, Accepted date: Apr 15, 2015, Publication date: Apr 20, 2015

Copyright: © 2015 Hai NV, et al. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

Abstract

The principles of linear accelerator are: the accelerator emits two types of radiation that are photon and electron. However, when we were doing the research and working on it, we have found that neutrons have emitted from the accelerator.

This paper aims to show some results of measuring neutrons from a linear accelerator at Dong Nai General Hospital. The results of this experiment will be used to ensure the safety of radiation as well as the background for the incoming research.

Keywords: Linac; Neutron activation; Radiation therapy

Introduction

Based on the theory, photons with energy which is greater than 6MV is able to generate a reaction (γ, n). This reaction depends on the material of target, it will create a beam of neutrons with considerable intensity. In order to measure this beam of neutrons, we have used a ALOKA dose meter.

However, the result hasn't been very reliable because the secondary radiations have taken part in the measuring process and this dose meter can measure the other radiations. Therefore, we have used the neutron activation method to measure and calculate the dose rate of neutron from Dong Nai General Hospital.


The Theory

When neutron with high energy- interacts with a nucleus target, two main processes that are elastic scattering and neutron capture reaction can occur.

In case neutron capture happens, a compound nuclear is generated with the stimulating energy equal to the combined energy between the neutron and the nuclear and kinetic energy of the incident neutron.

The compound energy exists in the simulating state during 10^{-14} s then it decays to basis state or ISOME state by radiating prompt gamma ray and forms radioactive nucleus with mass number equal to $A+1$. Most of the nucleus are unstable and decay to a new nuclear by emitting beta and gamma ray called delayed gamma ray.

The process of activation by neutron capture reaction is illustrated in Figure 1.

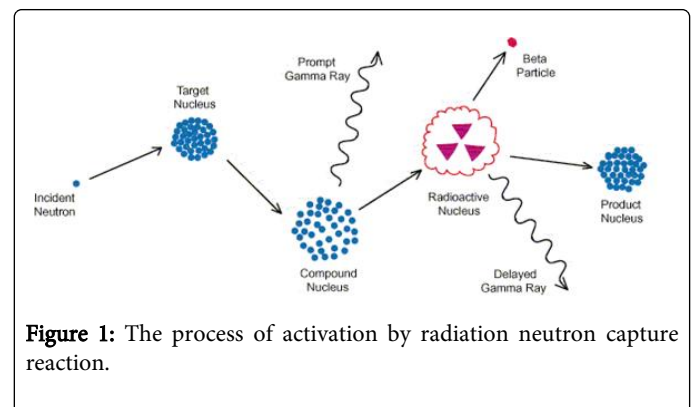

By using samples of standard target nucleus is exactly known as element content, quantity of samples, the common of isotope, geometry of samples, cross section of radiation-capture and measuring delayed gamma spectrometry from radioactive nucleus with multi-channel spectrometer-HPGe. The information on neutron flux density at the position of the samples will be determined accurately [1-4].

Carrying Out the Experiment

To obtain the accurate and reliable results, it is necessary to limit the error sources which can contribute to the measurement results. Therefore, the samples are used in experiments must meet certain requirements as follows:

- The samples must have high purity.
- The samples must have stable chemical composition, it is best to use metal.
- Samples must have thin thickness in order that the self-shielding effect is negligible. The sample is considered thin is: $(\Sigma_a + \Sigma_s) \cdot d \ll 1$

in which $\Sigma_a + \Sigma_s$ is called macro cross section absorption and macro scattering for neutrons, ($\Sigma_a = N\sigma_a$), N: number of nuclears in 1 cm³, σ_a micro cross section absorption and scattering for neutrons, we defined Σ_s similarly.

- Resonance energy and energy thresholds in the different reactions should have good distance.
- Nuclear product obtained after activation with the following characters:

+suitable half-life.

+A known simple decay scheme

+emitting gamma radiation without interference from radiation background of surroundings.

From the above criteria, we choose gold (¹⁹⁷Au) as a sample with diameter 1.27 mm, 0.05 mm thick, for these experiments. The image of the gold samples is illustrated as the Figure 2. The characteristics of gold is presented in Table 1. In that table we show characteristics of ¹⁹⁷Au, and ¹⁹⁸Au (Radioactive nuclues) [4-6].



Figure 2: Samples ¹⁹⁷Au used in the experiments.

Nuclear	Popularity θ(%)	σ_a (barn)	Product of activation	T _{1/2}	E _γ (keV)	γ(%)
¹⁹⁷ Au	100	98.8	¹⁹⁸ Au	2,69 5	411	95

Table 1: Characteristics of samples ¹⁹⁷Au.

The process of sample preparation: Cleaning by alcohol → drying → weighing to define the mass with electronic scale, the accuracy is 0.0001 gram. The sample is put into a container. Then it will be taken to the Hospital in order to be attached to the positions as presented in Figure 3.

The distance from the Hospital to the location with the delayed gamma spectrometer is 200 km and the time of moving is 8 hours. On the other hand, the Hospital only can use radioactive therapy for 2 hours/ day (depending on the patient) (Table 2). Therefore, we only carry out the process of neutron activation during 2 hours, but the time emit only 20 minutes. After that, we carry out the measuring process, we have done to bring the sample to analyze, calculate flux of delay by Gamma spectrometer in Figure 4 software gamma vision at Figure 5 [5].

The most important aim in this paper is investigation neutron inside treatment room, therefore the result just only care about dose rate of neutron, don't discriminate between neutrons.

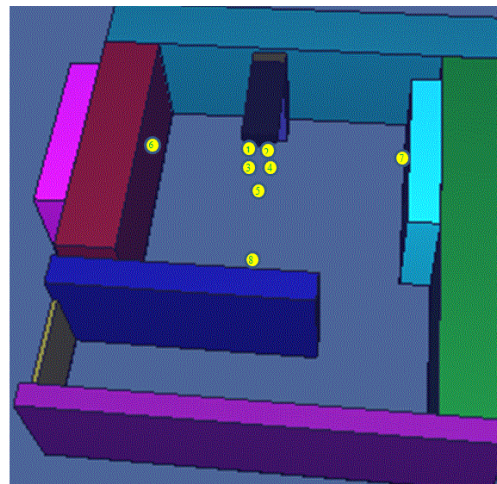


Figure 3: Positions of attached samples.

Position	1	2	3	4	5	6	7	8
Name samples	Au-Lx4	Au-Lx2	Au-Lx6	Au-Lx3	Au-VN5	Au-Lx5	Au-Lx1	Au-Lx7

Table 2: The position corresponding to the activated sample.



Figure 4: Spectrometer used in experiments.

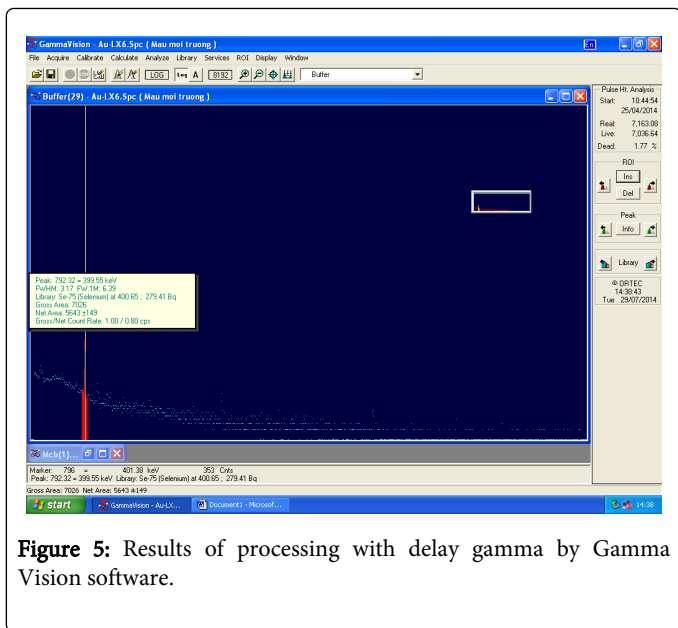


Figure 5: Results of processing with delay gamma by Gamma Vision software.

6×10^7	4.4	-
10^8	5.6	-

Table 3: The exchange coefficient from flux to dose rate per 1 mrem/hour unit of dose rate with defireency neutron Energy.

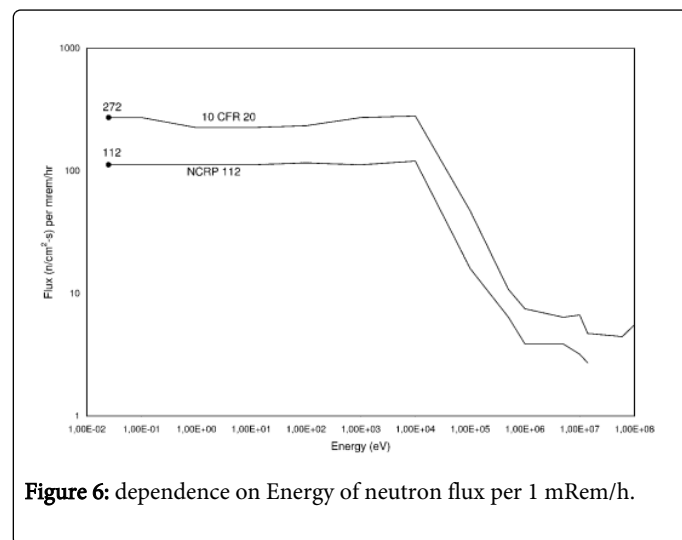


Figure 6: dependence on Energy of neutron flux per 1 mRem/h.

Result and Discussion

Results of the analysis, process, calculate. We obtained neutron flux at the positions in the radiation therapy room (Figure 4). These results demonstrate the generation of great amounts of neutron radiation therapy room (Table 3).

To determine dose rate of neutron from flux of neutron: Dose rate of neutron can determine from results calculation flux by using International standard about exchange coefficient from flux to dose rate (Table 4). Two populer standards using now are: 10CFR (US Nuclear Regulatory Commission) and another one is NCRP (National Council on Radiation Protection and Measurement) (Figure 6) [4,6].

Neutron (eV)	Neutron Flux (n/cm ² s) per 1 mRem/h	
	10CFR 20	NCRP 112
0.025	272	112
0.1	272	112
1	224	112
10	224	112
10 ²	232	116
10 ³	272	112
10 ⁴	280	120
10 ⁵	46.0	16.0
5x10 ⁵	10.8	6.40
10 ⁶	7.6	3.88
5x10 ⁶	6.4	3.88
10 ⁷	6.8	3.20
1.4x10 ⁷	4.8	2.72

Name of Sample	Start to mount	Stop to mount	Total	Time mesuarments (s)	Flux of neutron	Dose rate mSv/h
Au-Lx5	04/23/14 08:00:00	04/23/14 08:20:00	1200	37782	15,153	1.39
Au- Lx6	04/23/14 08:00:00	04/23/14 08:20:00	1200	7036	23,524	2.16
Au-Lx7	04/23/14 08:00:00	04/23/14 08:20:00	1200	8801	7,795	0.72
Au- VN5	04/23/14 08:00:00	04/23/14 08:20:00	1200	11803	10,603	0.97
Au-Lx1	04/23/14 08:00:00	04/23/14 08:20:00	1200	8159	5,210	0.48
Au-Lx2	04/23/14 08:00:00	04/23/14 08:20:00	1200	2370	8,485	0.78
Au Lx3	04/23/14 08:00:00	04/23/14 08:20:00	1200	8201	6,335	0.58
Au- Lx4	04/23/14 08:00:00	04/23/14 08:20:00	1200	3392	5,295	0.49

Table 4: Neutron dose rate in positions of the radiation therapy room.

Weigh Radiation of neutron very high, so it damages for tissue of patients. And it contribute to total of dose. Therefore, to ensure safety during and after the treatment we recommend:

- There are specific calculations of dose distributions produce neutrons in radiotherapy rooms with great projects and conduct done with most of the hospitals.

- On the basis of these research results, we must to conculcate for shielding to ensure the safety of patients. It will be to make important basis to cater for the old hospital and new hospital.

References

1. Ngo Quang Huy (2006) Base on nuclear physics. Science and Technical publish.
2. http://www.unimasr.net/ums/upload/files/2011/Dec/UniMasr.com_c2ee784814d50b7354a490bce4424a6d.pdf.
3. [No authors listed] (1999) Radiation Protection Distance Learning. Australian Nuclear Science & technology Organization. Sydney, Australia.
4. Herman Center (1996) "Introduction to health Physics". The McGraw Hill Copmanies, Inc.
5. Lin SY, Chu TC, Lin JP (2001) Monte Carlo simulation of a clinical linear accelerator. Appl Radiat Isot 55: 759-765.
6. Omrane LB Verhaegen F, Chahed N, Mtimet S (2003) An investigation of entrance surface dose calculations for diagnostic radiology using Monte Carlo simulations and radiotherapy dosimetry formalisms. Physics in Medicine and Biology 48: 1809-1824.